

Multidrug Resistance Activity Kit

Kit Contents

Name	Volume	Containers	Storage
4 mM Calcein AM in DMSO	50 μ L	2	-20° C
1000X Cyclosporine A in Ethanol	50 μ L	1	-20° C
1X Assay Buffer, pH 7.3	100 mL	1	RT
TRS	4 mL	1	RT

Description

ION's Multidrug Resistance (MDR) Activity kit is an effective solution for detecting MDR1 and MRP1 activity and compounds susceptible to MDR-mediated efflux. ION's MDR Activity kit is compatible with fluorescence microscopy, flow cytometry, and fluorescence plate readers using FITC/fluorescein settings.

Calcein AM is a membrane-permeant, non-fluorescent dye that enters cells passively. Once inside the cytosol of cells, intracellular esterases convert it to fluorescent Calcein (Ex/Em: 495 nm/515 nm), resulting in uniform cytosolic fluorescence. Drug efflux transporters, such as P-glycoprotein (Pgp, MDR1) and multidrug-resistance-associated protein (MRP1), actively extrude Calcein AM from inside the cell before esterases can convert it to Calcein. The presence of additional MDR substrates or inhibitors of MDR expression results in decreased Calcein AM efflux, causing a measurable increase in intracellular fluorescence. In addition to identifying MDR substrates and inhibitors, this kit can also be used to evaluate the activity of MDR transporters in cells.

When following our protocol, ION's MDR Activity kit provides enough reagents to make 100 mL of working solution, enough for ten 96- or 384-well plates or 80 flow cytometry samples. The actual number of assays will vary according to optimal dye concentrations for your application.

Laboratory Procedures

Getting Started

Before you begin, make sure that you have all the additional reagents and materials you will need for the successful completion of your experiment. Although ION's MDR Activity kit contains the key reagents you will need to prepare your cells for analysis, your experiments will likely require other reagents which are not included in your MDR Activity kit. Notably, compounds to be tested, buffers and solvents for the dissolution of these compounds, and reagents necessary for cell culture are not included.

In addition to reagents - a microscope, fluorescence plate reader, or flow cytometer that is capable of providing an excitation source at ~ 495 nm and measuring emission at ~515 nm is required. Compatible filters are FITC or GFP.

General Considerations

1. Optimal Calcein AM concentrations will vary depending on cell type and application. Recommended Calcein AM concentrations range between 1 μM and 2 μM .
2. Minimize freeze-thaw cycles of Calcein AM and Cyclosporine A solutions.
3. Aqueous solutions of Calcein AM are susceptible to hydrolysis; therefore, all working solutions should be used as quickly as possible and no later than 4 hours after preparation.
4. Calcein cannot withstand fixation after staining.
5. Serum-containing solutions may increase extracellular fluorescence. If conducting an assay with serum present, we recommend including TRS to minimize extracellular fluorescence.
6. Cyclosporine A can be used as a positive control. Use at a concentration of 5 μM (1:1000 dilution) for maximum efficacy.
7. Molecules that affect esterase activity, intracellular ATP production, or that bind to alternative MDR binding sites may result in an inaccurate classification of MDR substrates.

Plate Reader Assay

1. For adherent cells, plate cells overnight, seed $\sim 30,000$ cells/well/100 μL in a 96-well plate or $\sim 10,000$ cells/well/25 μL in a 384-well plate. When using this assay kit, make sure to use cells that possess high levels of MDR activity such as CHO K1, HCT-8, U2OS, or cells that have been genetically engineered to overexpress MDR proteins.
2. Remove one vial of Calcein AM and 1000X Cyclosporine A from freezer and allow to warm to room temperature. Protect reagents from light.
3. Prepare the test compound solutions at the desired concentrations in buffer of choice (HBSS or HHBSS).
4. For a positive control, make the appropriate amount of Cyclosporine A solution needed, enough for 100 μL /well to be evaluated. For example, add 1 μL of 1000X Cyclosporine A solution to 0.999 mL of the buffer used in **step 3**.
5. Remove medium from the wells of the plate and add 100 μL /well of test compound solutions, including your positive control solution from **step 4**. Incubate for 15 - 30 minutes at 37 $^{\circ}\text{C}$ or room temperature.
6. Prepare **dye loading solution** that contains 2X Calcein AM, 4 μM (1:1000 dilution) in 1X Assay Buffer. For example, add 10 μL of Calcein AM to 10 mL of 1X Assay Buffer for a full plate. Vortex briefly to mix.
7. Optional: Add 400 μL of TRS to the **dye loading solution**. Adjust 1X Assay Buffer volume in **step 6** to 9.6 mL. TRS minimizes extracellular fluorescence and is recommended when long incubation times with **dye loading solution** or serum containing media are used.
8. After the 15 - 30 minute incubation period from **step 5** is complete, add **dye loading solution** prepared in **step 6/7** directly to wells. Add 100 μL /well to a 96-well plate.
9. Incubate cells for an additional 30 minutes at 37 $^{\circ}\text{C}$ or room temperature. Protect from light.
10. Measure fluorescence using a fluorescence plate reader. For Calcein, use Ex/Em ~ 495 nm/515 nm or FITC settings.

*Note: If conducting an assay using a fluorescence microscope, use GFP or FITC filters to acquire images. If using non-adherent cells, follow flow cytometry protocol until **step 10**. Then add cell suspensions to wells of a microplate and centrifuge your plate before acquiring fluorescence data.

Flow Cytometry Assay

1. Remove one vial of Calcein AM and 1000X Cyclosporine A from freezer and allow to warm to room temperature. Protect reagents from light.

- Prepare your test compounds at the desired concentrations in 1 mL of the buffer of your choice (HBSS or HHBSS). To prepare the positive control, add 1 μL of the 1000X Cyclosporine A solution to 0.999 mL of the same buffer.
- If using adherent cells, detach cells from the culture dish and suspend cells in cell culture medium at a concentration of $\sim 1\text{-}2 \times 10^6$ cells/mL. For non-adherent cells, suspend in medium at your desired cell concentration.
- Prepare tubes for each assay condition in triplicate by adding 250 μL of the cell suspension from **step 3** to a minimum of 3 tubes. Add an extra tube for an unstained cell control, if desired.
- Centrifuge cells and remove the medium.
- Resuspend a single tube of cells in 125 μL of test compound solution or positive control solution. Repeat in triplicate (3 tubes total) for each test compound. Also include a vehicle control condition of 125 μL of your buffer containing the same DMSO concentration as your test compound solutions.
- Incubate tubes for 15 - 30 minutes at room temperature.
- During incubation period, prepare a **dye loading solution** that contains 2X Calcein AM, 4 μM (1:1000 dilution) in 1X Assay Buffer. For example, add 10 μL of Calcein AM to 10 mL of 1X Assay Buffer. Vortex briefly to mix.
- After the 15 - 30 minute incubation period from **step 7** is complete, add 125 μL of **dye loading solution** prepared in **step 8** to each tube.
- Incubate cells for an additional 30 minutes at room temperature. Protect from light.
- After the completion of **step 10**, centrifuge cells and aspirate your **dye loading solution** and test compound buffer. Resuspend cells in your preferred flow cytometry (FACS) buffer.

Example Results

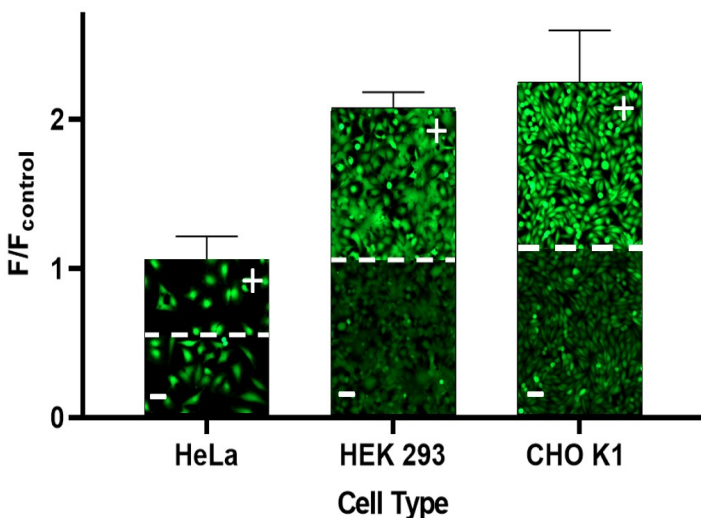


Figure 1. Calcein fluorescence in HeLa, HEK 293, and CHO K1 cells in the presence (+, top half of bar) or absence (-, bottom half of bar) of $\sim 5.0 \mu\text{M}$ CsA. Cells that do not express the transporter, such as HeLa cells, do not show a change in fluorescence when CsA is added. Fluorescence (Ex: 495 nm, Em: 515 nm) was recorded on a BioTek® Cytation 5 plate reader. Images were acquired using GFP filters, Ex: 469/35 nm, Em: 525/39 nm, and 4X objective on a BioTek® Cytation 5. Reported ratios are calculated using fluorescence “bottom-read” data. Error bars represent standard deviation.

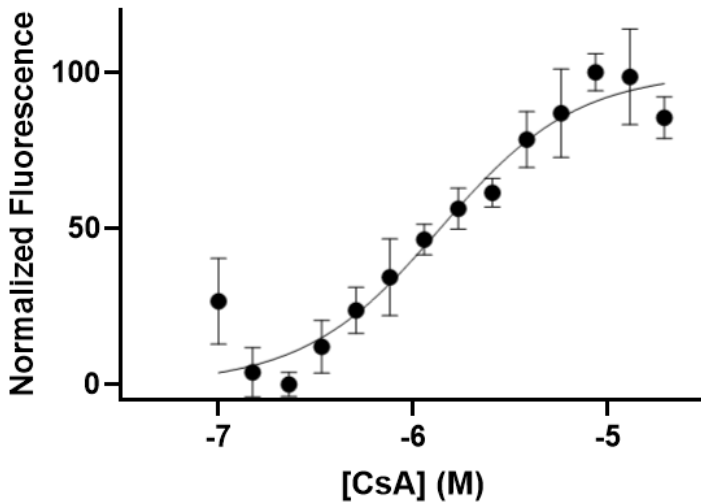


Figure 2. Cyclosporine A (CsA) dose response curve generated from fluorescence data collected from CHO-K1 cells. Fluorescence (Ex: 495 nm, Em:515 nm) was recorded on a BioTek® Cytation 5 plate reader. Cells were incubated with Cyclosporine A for 30 min at 37 °C. Calcein was then added and cells were incubated for another 30 minutes at 37 °C. The estimated EC₅₀ is 1.36 μM.

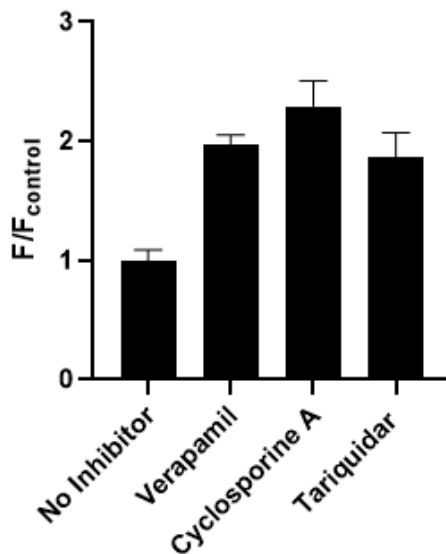


Figure 3. Fold change in fluorescence with the application of three different MDR1 inhibitors to CHO K1 cells. Verapamil is a non-competitive inhibitor of Pgp. Cyclosporine A is a competitive inhibitor on the Calcein AM binding site of Pgp. Tariquidar is a non-competitive inhibitor, as it inhibits substrate binding and ATP hydrolysis on Pgp. Cells were incubated with the inhibitors for 30 min at 37 °C. Calcein was then added and cells were incubated for another 30 minutes at 37 °C. Fluorescence (Ex: 495 nm, Em: 515 nm) was recorded on a BioTek® Cytation 5 plate reader.

References

1. Eilers M, et. al. [MRP \(ABCC\) transporters-mediated efflux of anti-HIV drugs, saquinavir and zidovudine, from human endothelial cells.](#) *Exp Biol Med (Maywood)*. (2008). 233(9).
2. Jakab K, et. al. [Application of flow cytometry immunophenotyping and multidrug resistance assay in B-cell acute lymphoid leukemia and multiple myeloma.](#) *Neoplasma*. (2005). 52(1).
3. Legrand O, et. al. [Pgp and MRP Activities Using Calcein-AM Are Prognostic Factors in Adult Acute Myeloid Leukemia Patients.](#) *Blood*. (1998). 91(12).
4. Ansbro MR, et. al. [Screening compounds with a novel high-throughput ABCB1-mediated efflux assay identifies drugs with known therapeutic targets at risk for multidrug resistance interference.](#) *PLoS One*. (2013). 8(4).

Related Products	
Product Code	Product Name
1071B	Calcein AM, Dry (1 mg)
1074	Calcein AM, 2 mM in DMSO (0.5 mL)
5000	ION Vital - Viability
5010	Ethidium Homodimer I, Dry (1 mg)
5020	Ethidium Homodimer I, 2 mM in DMSO (0.5 mL)